

10061879 "DEE102"

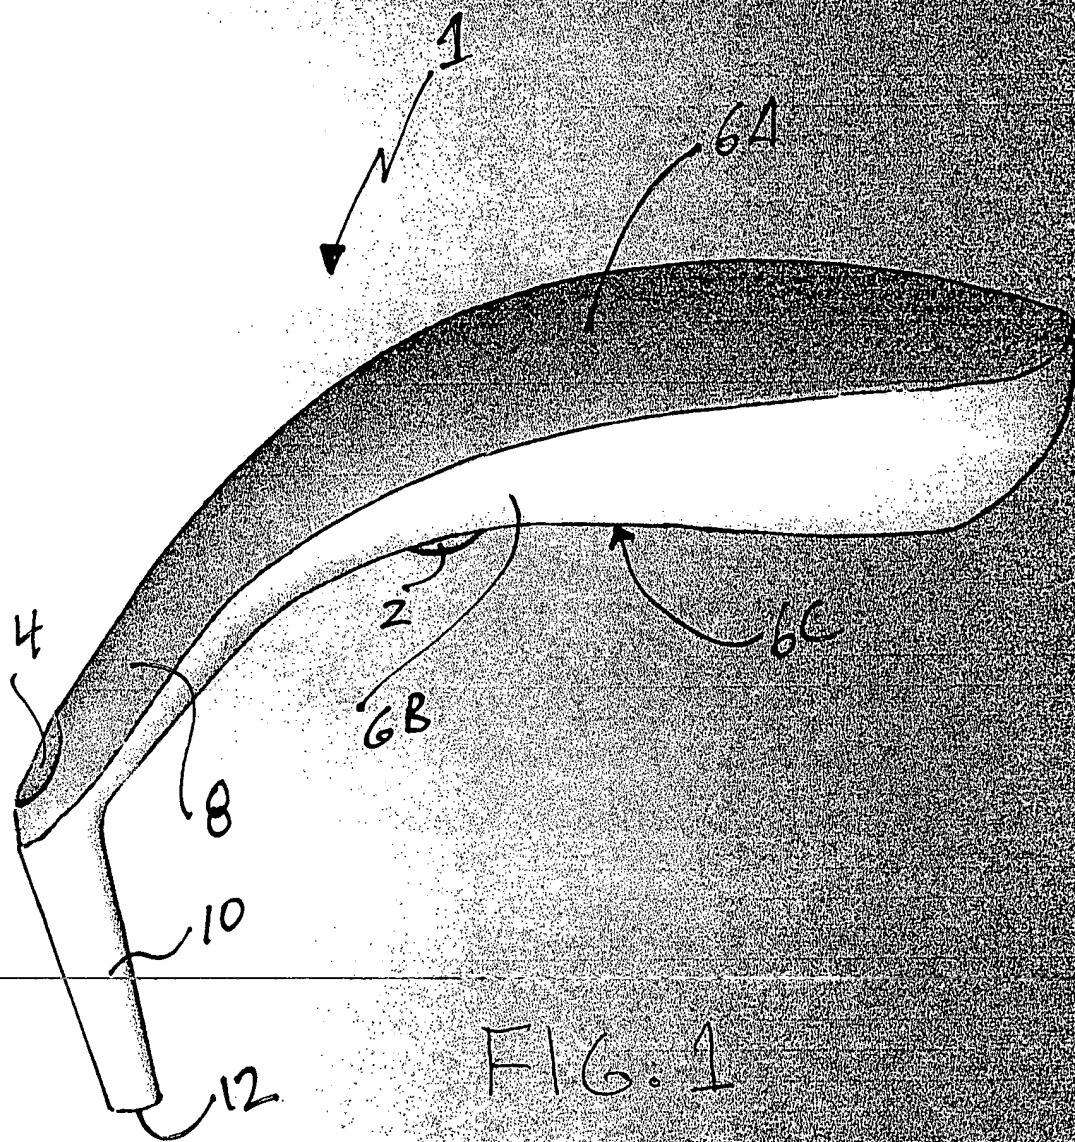


FIG. 1

10081879.022106

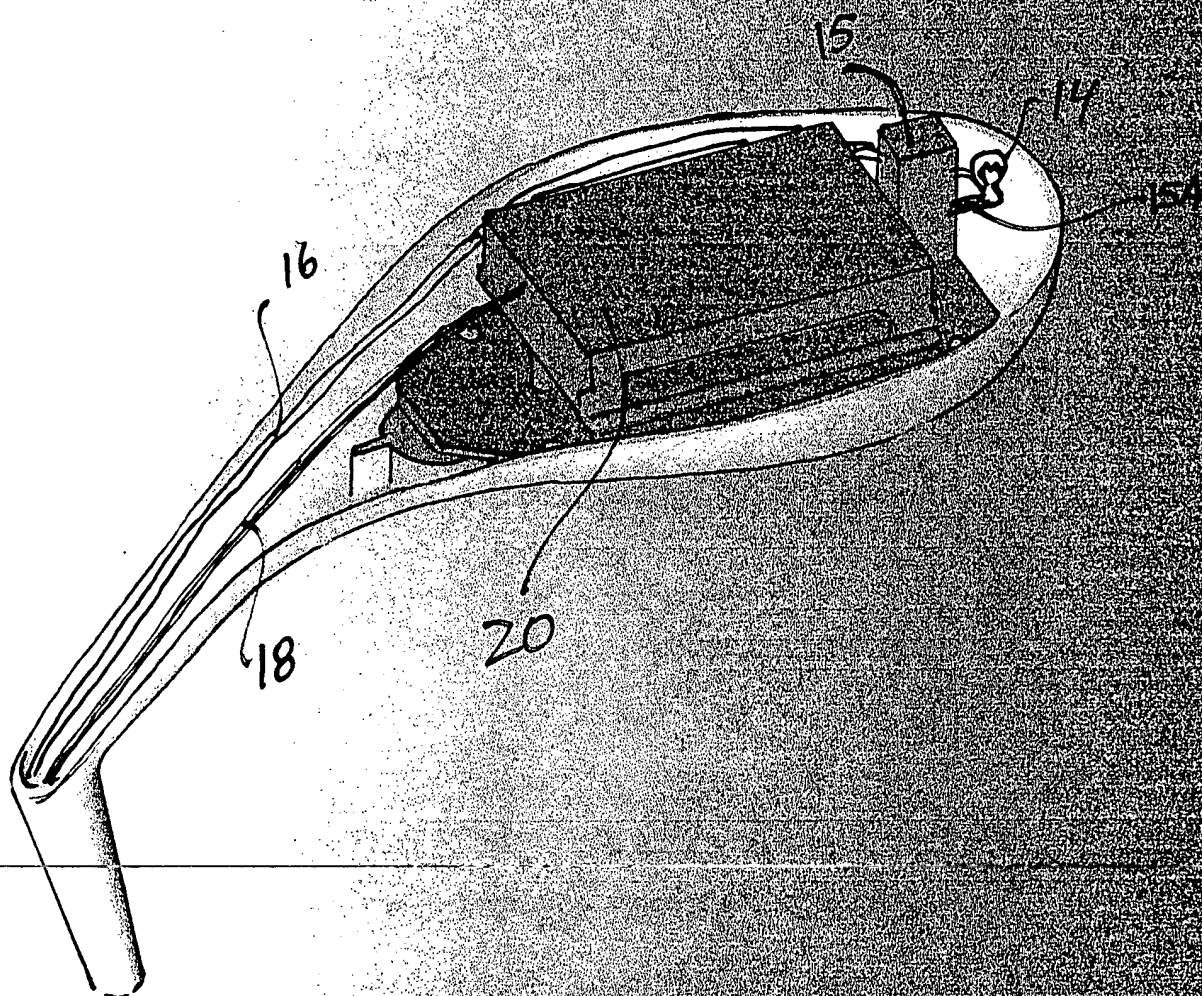


FIG. 2


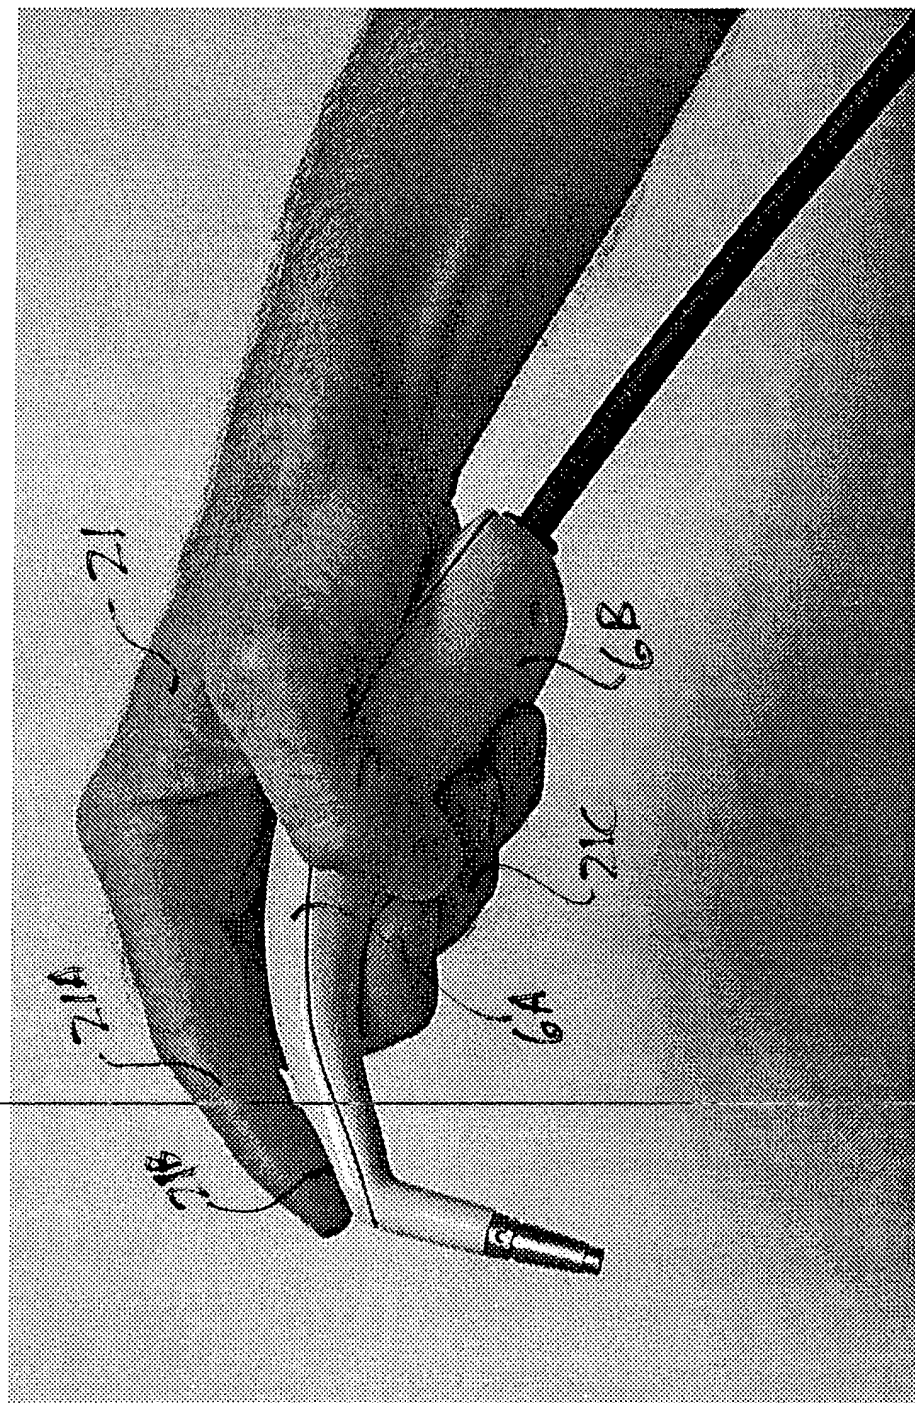


FIG. 3

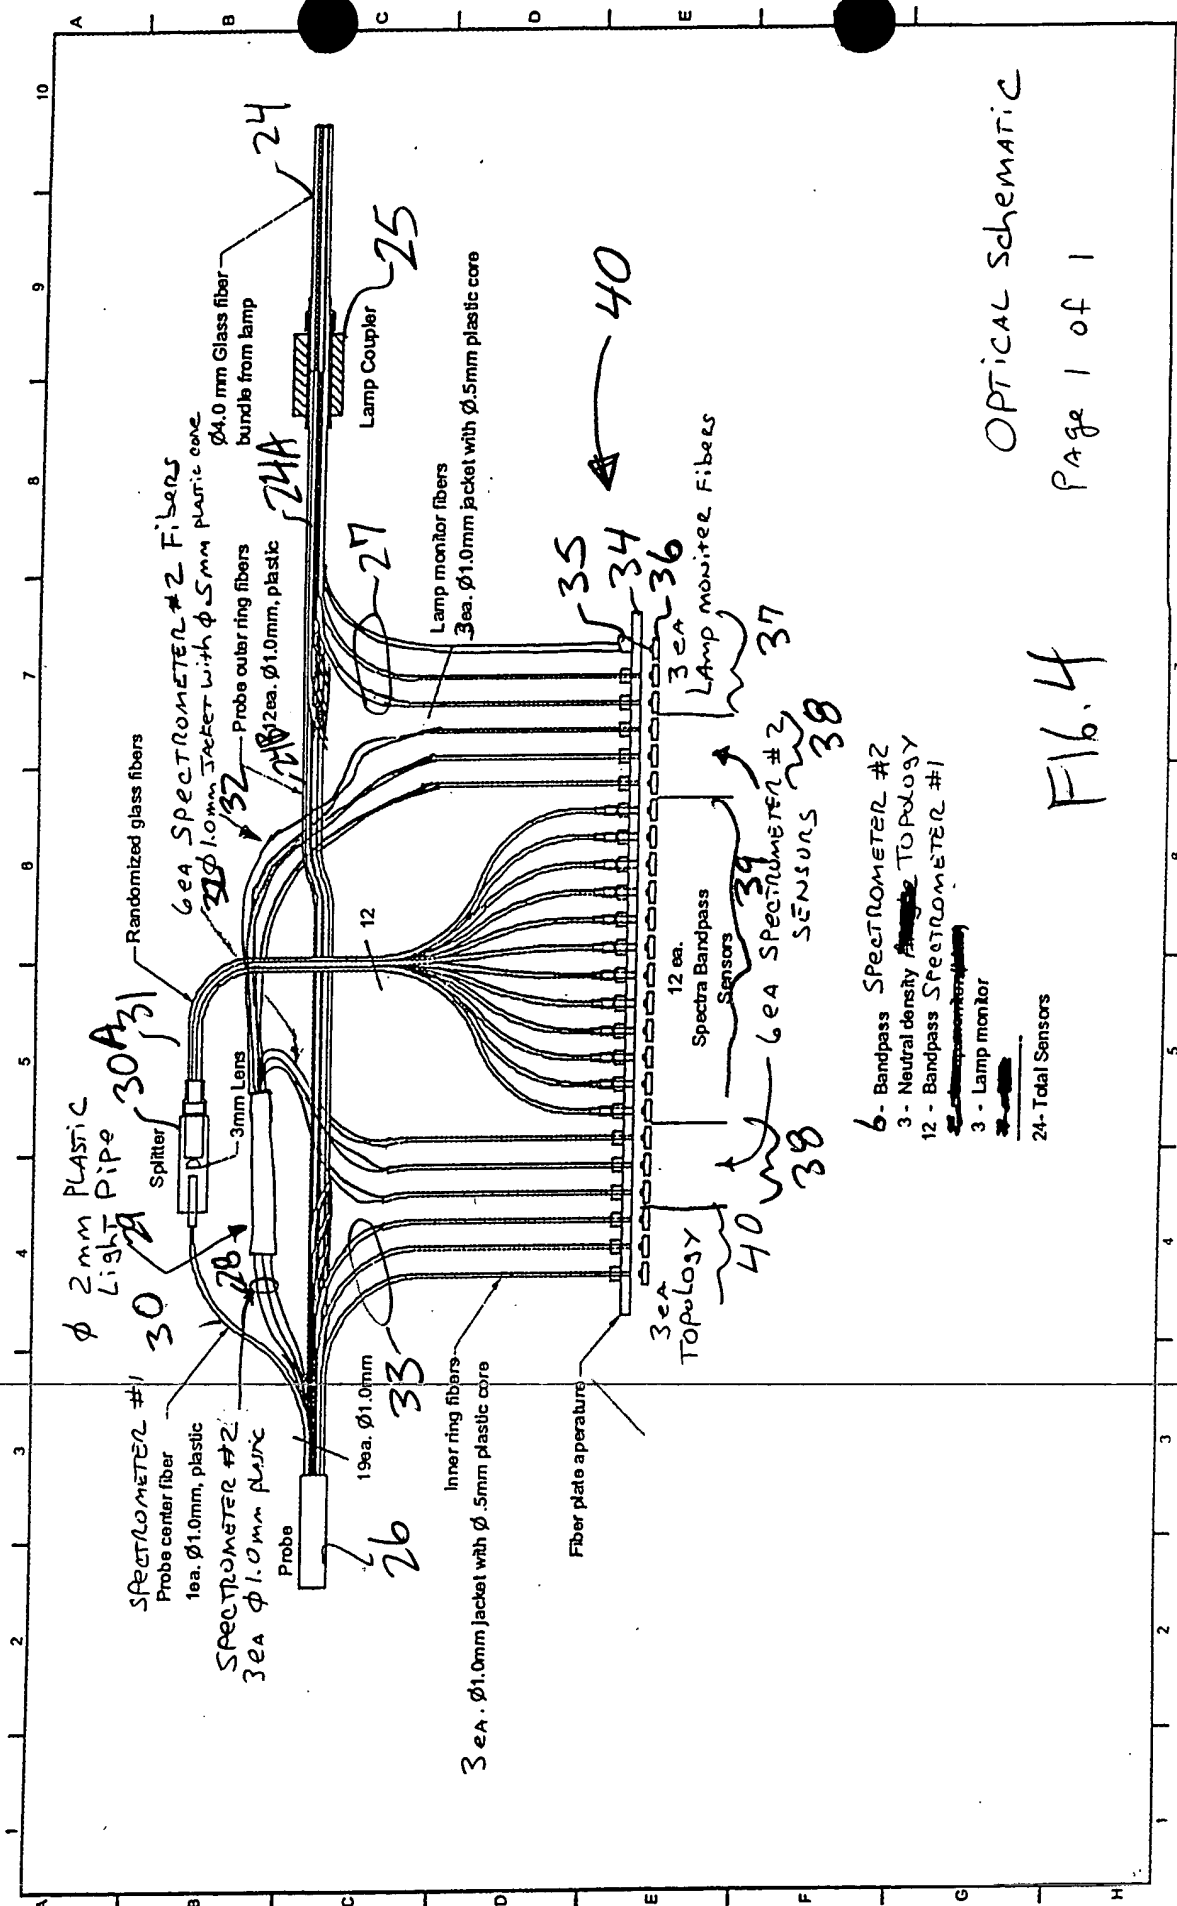

OPTICAL SCHEMATIC
Page 1 of 1

F16.4

- 6 - Bandpass Spectrometer #2
- 3 - Neutral density ~~filter~~ topology
- 12 - Bandpass Spectrometer #1
- 3 - Lamp monitor
- 24 - Total Sensors

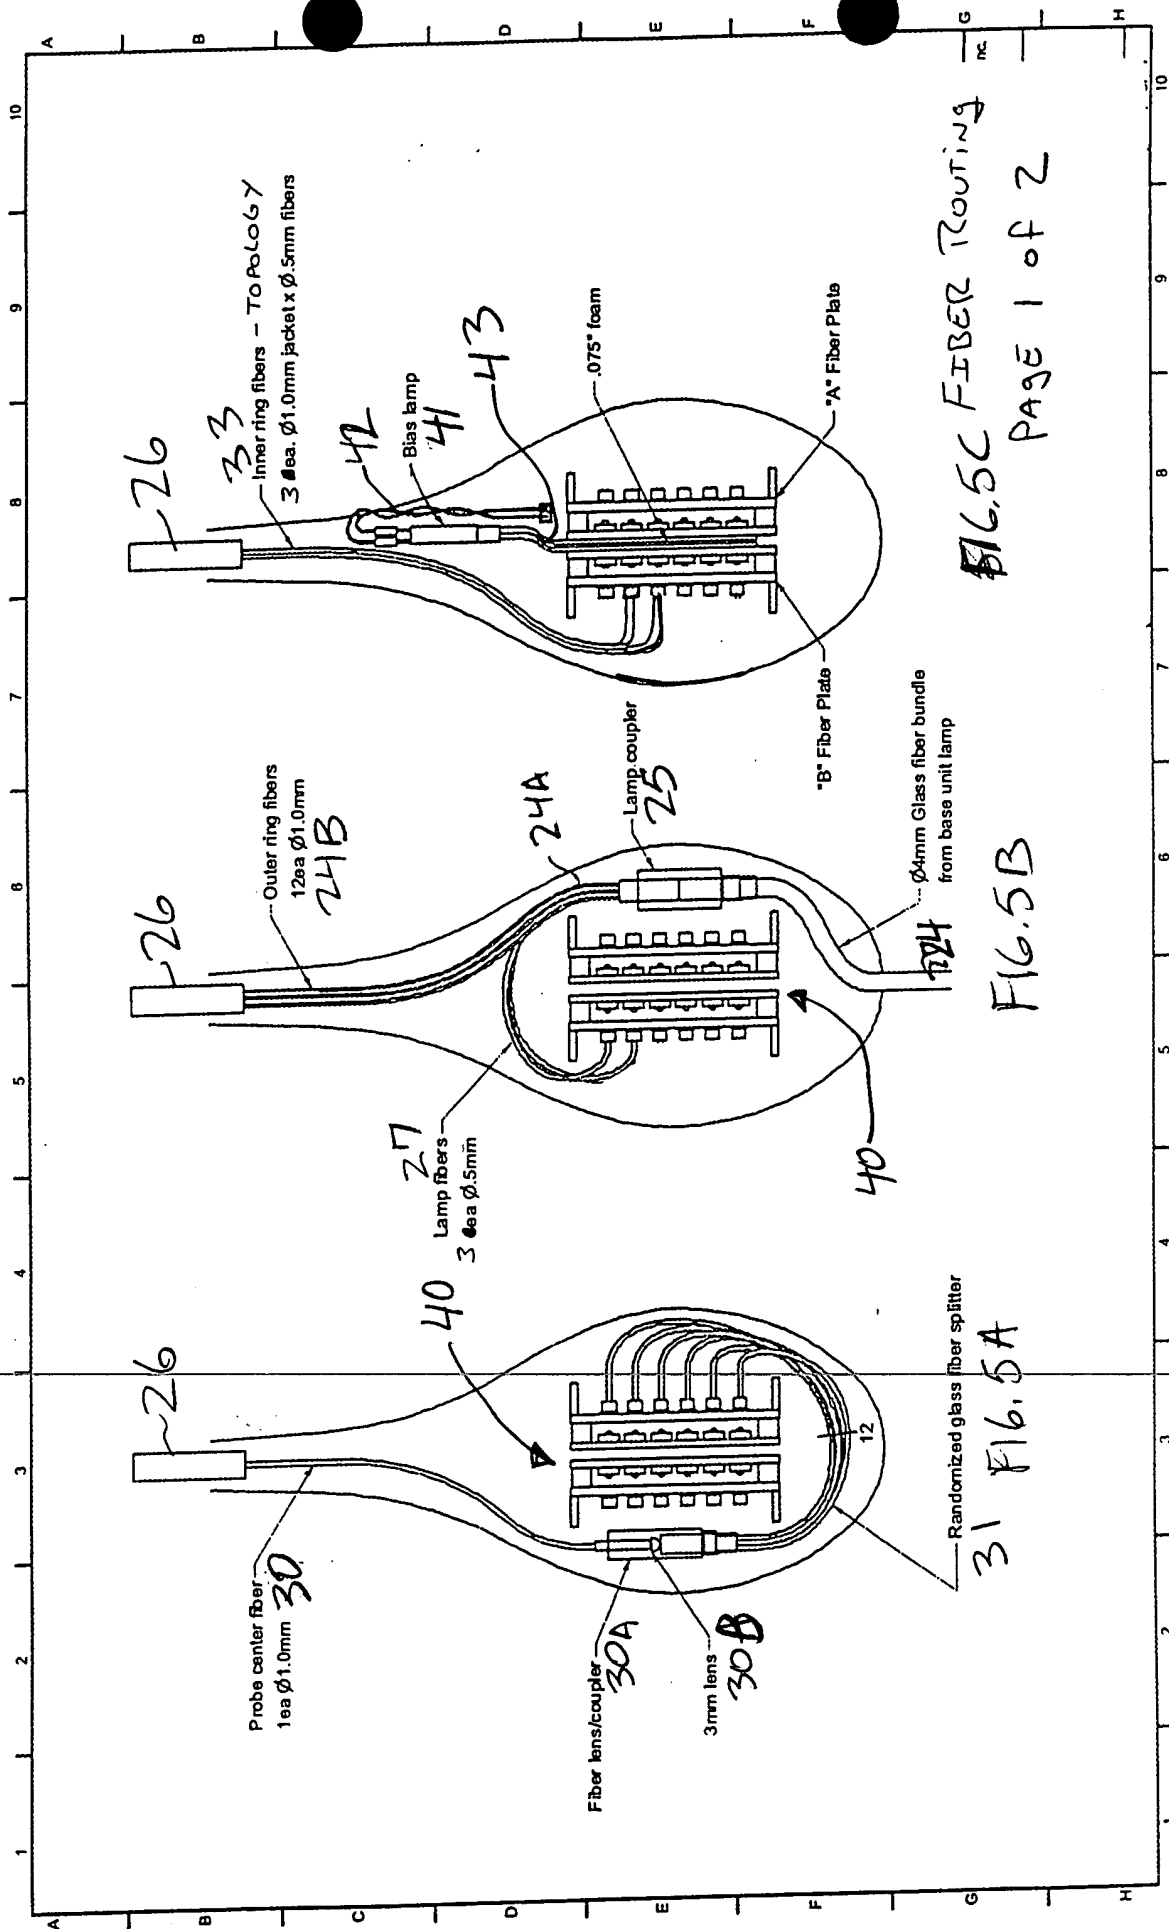


FIG. 5C FIBER ROUTING
PAGE 1 of 2

FIG. 5B

FIG. 5A

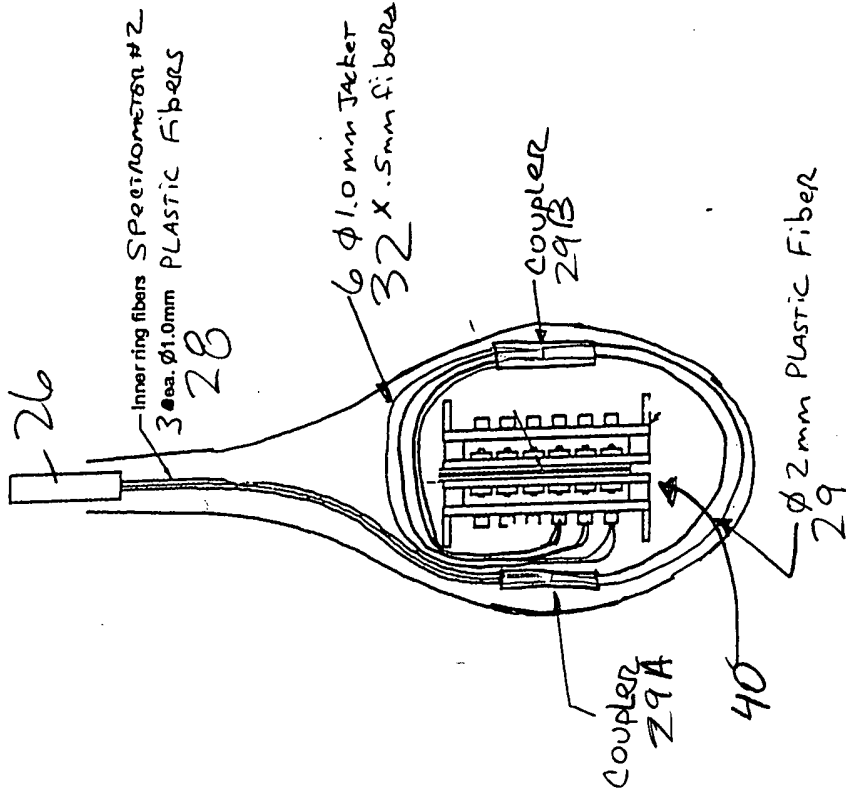


Fig. 5D
Fiber Routing
Page 2 of 2

Probe End View

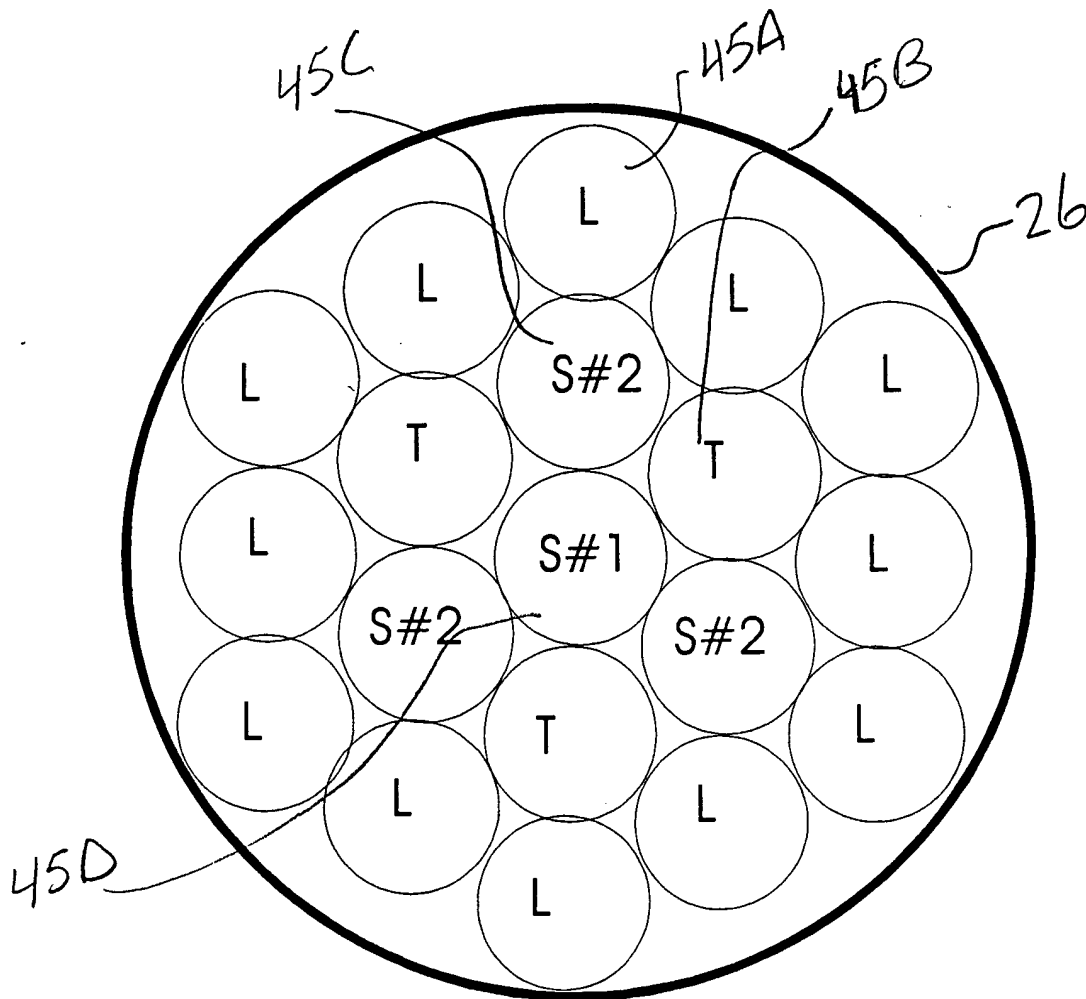


FIG. 6

L = Light Source

T = Topology

S #1 = Spectrometer #1 fiber

S #2 = Spectrometer #2 fibers

10061679 "DEP. 10"

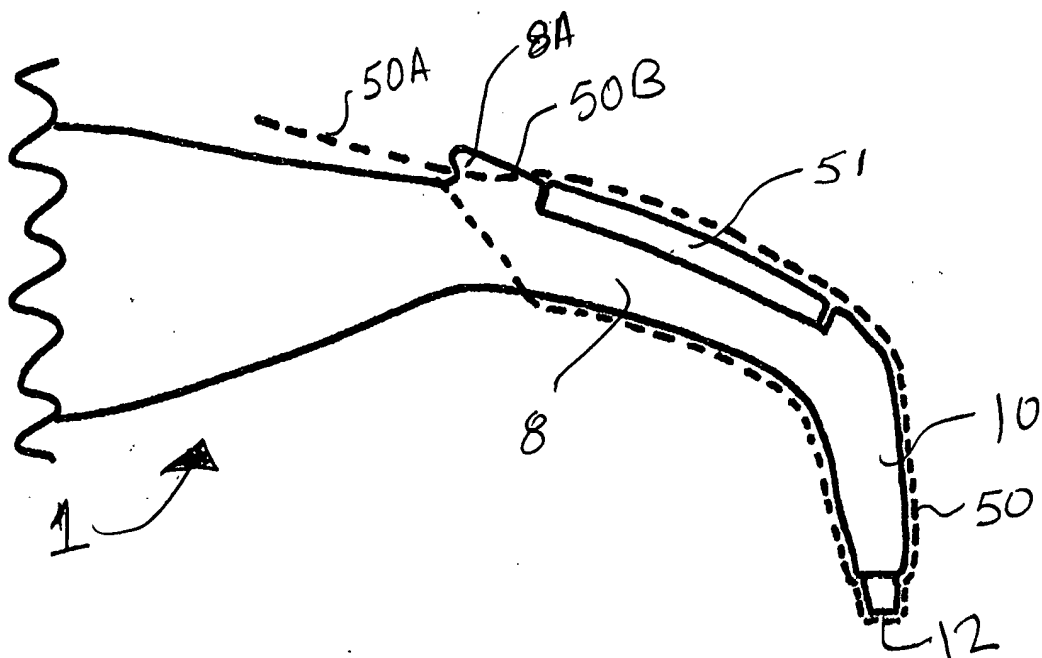


FIG. 7A

10081879.002103

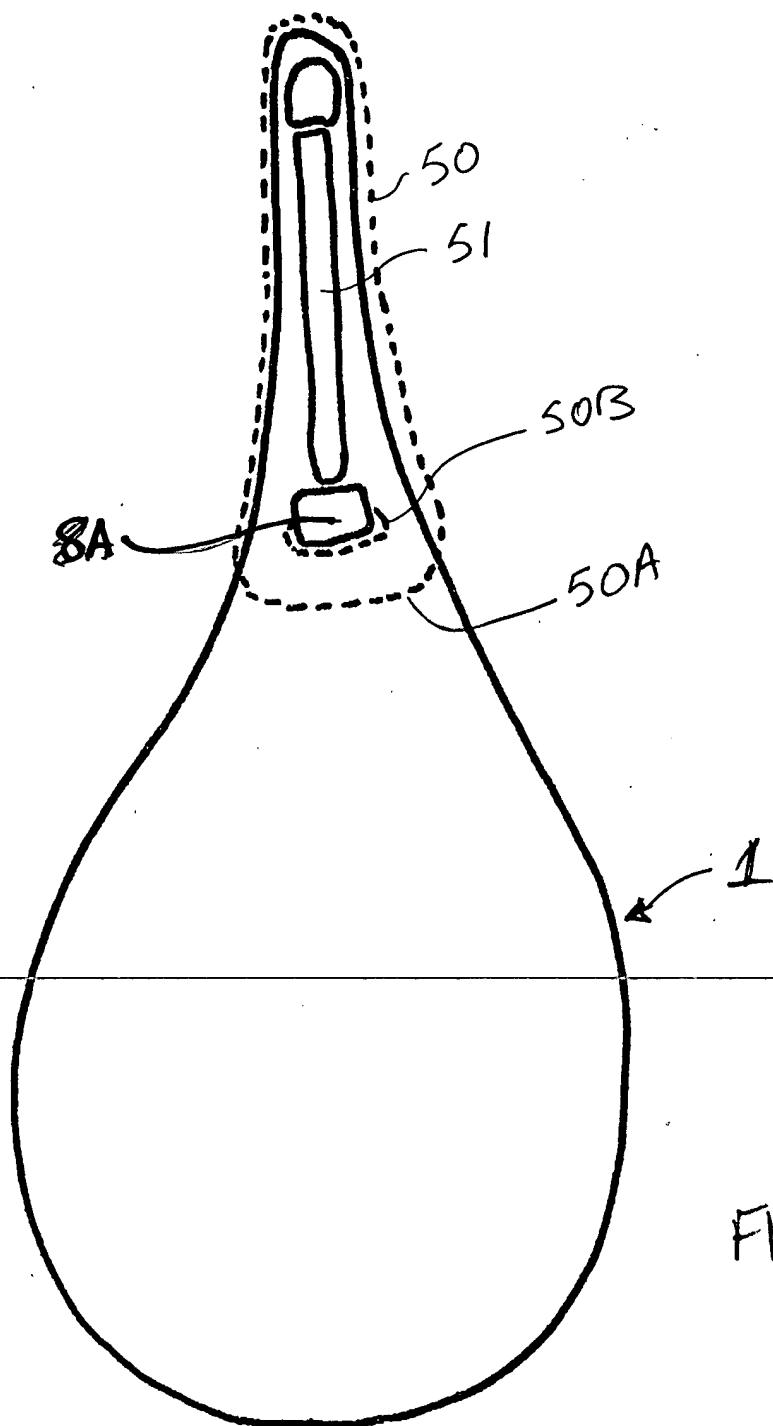


FIG. 7B

Year	1990	1991	1992	1993	1994	1995	1996	1997	1998	1999	2000	2001	2002	2003	2004	2005	2006	2007	2008	2009	2010	2011	2012	2013	2014	2015	2016	2017	2018	2019	2020	2021	2022	2023	2024	2025	2026	2027	2028	2029	2030	2031	2032	2033	2034	2035	2036	2037	2038	2039	2040	2041	2042	2043	2044	2045	2046	2047	2048	2049	2050	2051	2052	2053	2054	2055	2056	2057	2058	2059	2060	2061	2062	2063	2064	2065	2066	2067	2068	2069	2070	2071	2072	2073	2074	2075	2076	2077	2078	2079	2080	2081	2082	2083	2084	2085	2086	2087	2088	2089	2090	2091	2092	2093	2094	2095	2096	2097	2098	2099	2100
1990	1991	1992	1993	1994	1995	1996	1997	1998	1999	2000	2001	2002	2003	2004	2005	2006	2007	2008	2009	2010	2011	2012	2013	2014	2015	2016	2017	2018	2019	2020	2021	2022	2023	2024	2025	2026	2027	2028	2029	2030	2031	2032	2033	2034	2035	2036	2037	2038	2039	2040	2041	2042	2043	2044	2045	2046	2047	2048	2049	2050	2051	2052	2053	2054	2055	2056	2057	2058	2059	2060	2061	2062	2063	2064	2065	2066	2067	2068	2069	2070	2071	2072	2073	2074	2075	2076	2077	2078	2079	2080	2081	2082	2083	2084	2085	2086	2087	2088	2089	2090	2091	2092	2093	2094	2095	2096	2097	2098	2099	2100	

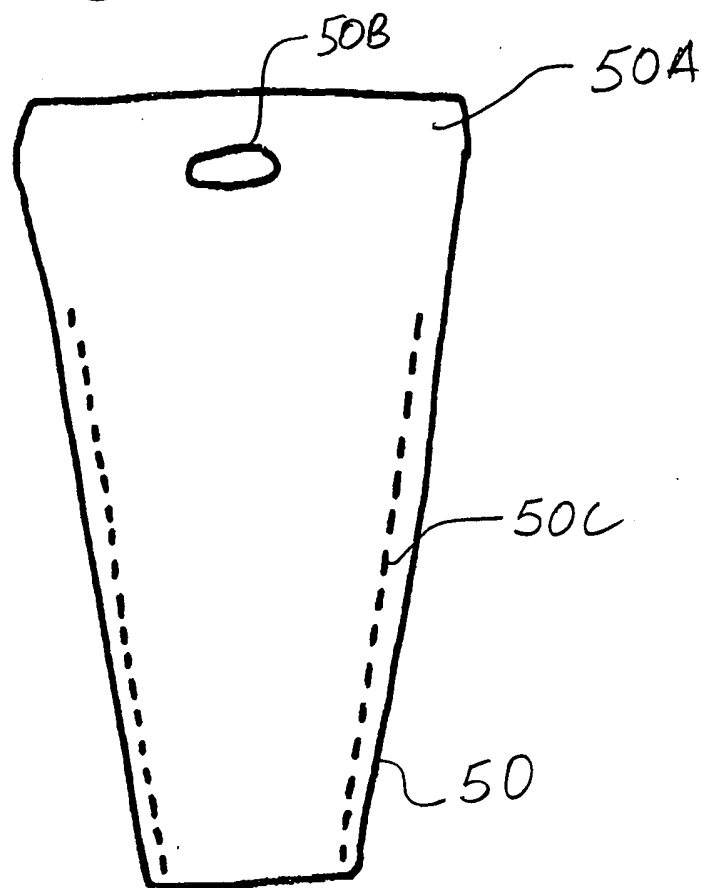


FIG. 7C

10081879.022102

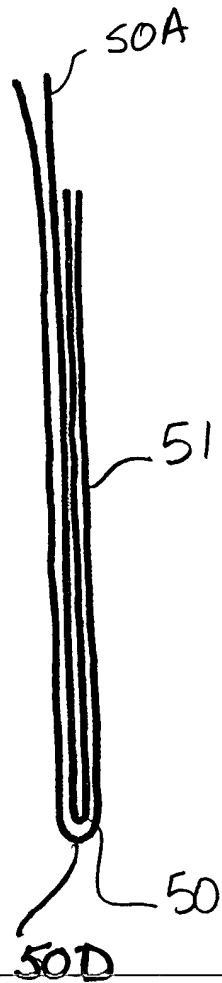


FIG. 7D

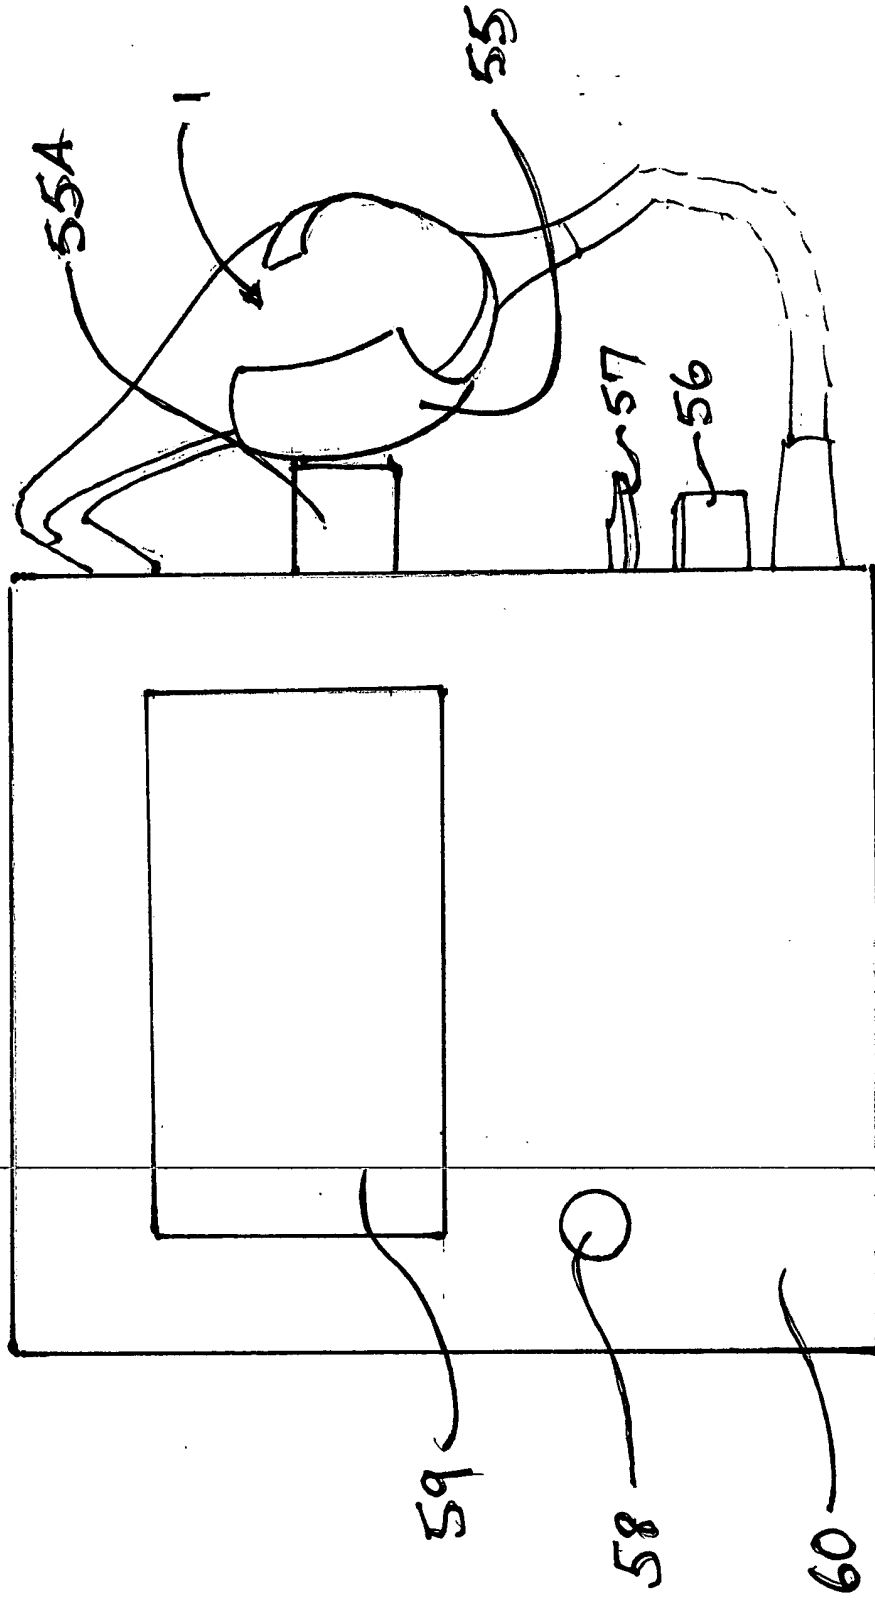


FIG. 8

FRONT WITH HANDPIECE

Easysshade®

Insert tip and
calibrate probe.

[Presets]

10081879 022103

FIG. 9A

Select

Tooth

Ceramic

Denture

Resin

20250101 10:20:00

Fig. 9B

Classical

3D Master

B1

2R1.5



1 Tooth 1

10081379 "022102

F16.9C

Classical

B 1


$\Delta E = 0.0$

$\Delta L = 0.0$

$\Delta C = 0.0$


2013015789001

F16. 9D

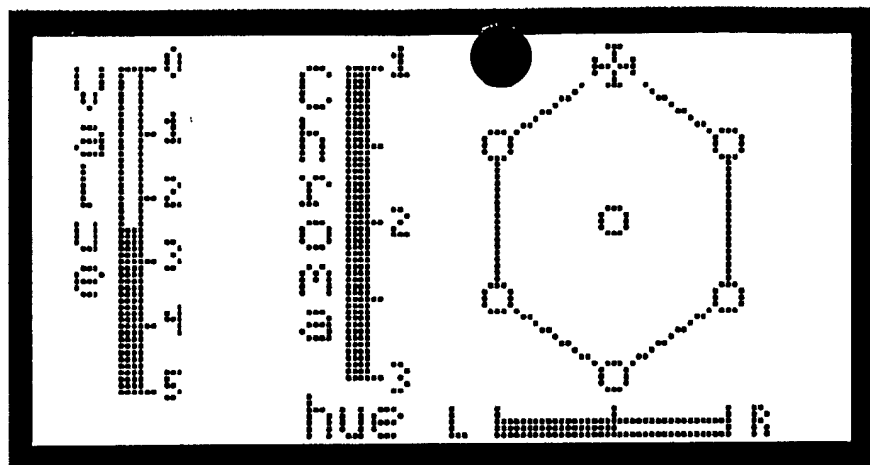


10061879-022102

F16.9E

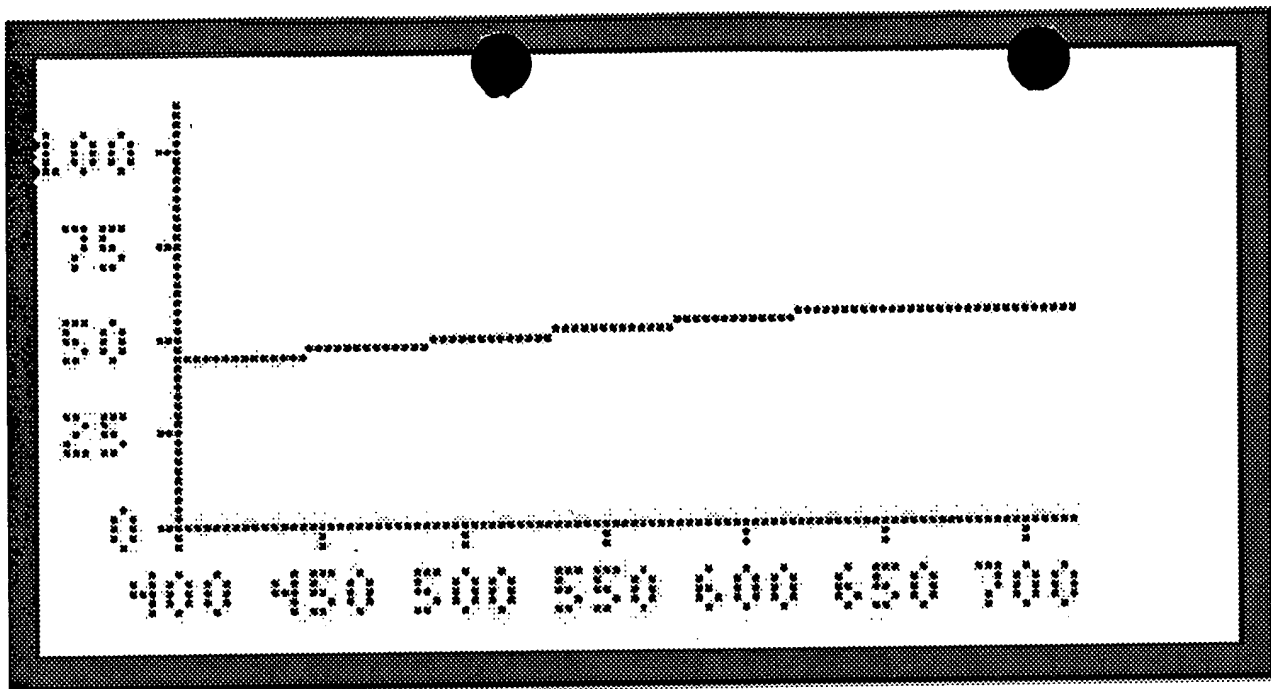

10081879-022102

Fig. 9 F

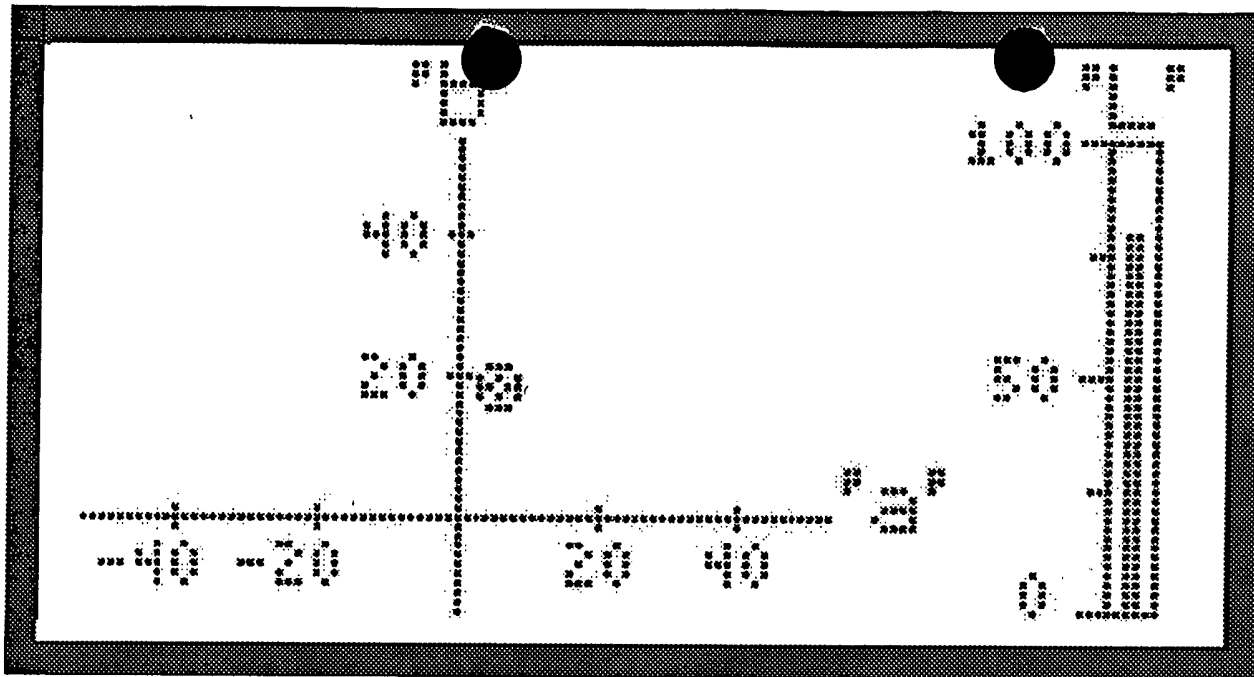

10081879 000100

Fig 9 G

文
明
之
光

2VB

52

THE

IM2

IM2

EMI

2R2.5

2M2

3R1.5

IM2

171

3L1.5

IM2

1M12

IMI

2MB

2R2

2MHI

FIG. 10